

Initial S™: Single use sterile kits for hand surgery

Initial S™ - Hand - Instrumentation kit content*

STERILE INSTRUMENTATION FOR Ø2.25 MM CANNULATED SCREWS

| Kit | Description | Content | Qty |
|-------------|---|--|-----|
| KIT-SC2.25H | Kit for Ø2.25 mm cannulated screws - Hand | Ø1.7 mm quick coupling drill bit - cannula Ø0.9 mm - L93mm | 1 |
| | | 3 in 1 instrument for Ø2.25 mm screws | 1 |
| | | Double guide Ø0.9 mm / Ø1.8 mm for Ø2.25 mm screws | 1 |
| | | 5.8 mm single use handle | 1 |
| | | Pin Ø0.8 L150 mm | 2 |
| | | Pin Ø0.8 L120 mm | 1 |

STERILE INSTRUMENTATION FOR Ø2.6 MM CANNULATED SCREWS

| Kit | Description | Content | Qty |
|------------|--|---|-----|
| KIT-SC2.6H | Kit for Ø2.6 mm cannulated screws - Hand | Ø2.0 mm quick coupling drill bit - cannula Ø1.1 mm - L93 mm | 1 |
| | | 3 in 1 instrument for Ø2.6 mm screws | 1 |
| | | Double guide Ø1.1 mm / Ø2.1 mm for Ø2.6 mm screws | 1 |
| | | 5.8 mm single use handle | 1 |
| | | Pin Ø1.0 L150 mm | 2 |
| | | Pin Ø1.0 L120 mm | 1 |

STERILE INSTRUMENTATION FOR Ø3.0 MM CANNULATED SCREWS

| Kit | Description | Content | Qty |
|------------|--|---|-----|
| KIT-SC3.0H | Kit for Ø3.0 mm cannulated screws - Hand | Ø2.2 mm quick coupling drill bit - cannula Ø1.1 mm - L93 mm | 1 |
| | | cannula Ø1.1 mm - L93 mm 1 | 1 |
| | | Double guide Ø1.1 mm / Ø2.3 mm for Ø3.0 mm screws | 1 |
| | | 5.8 mm single use handle | 1 |
| | | Pin Ø1.0 L150 mm | 2 |
| | | Pin Ø1.0 L120 mm | 1 |

Indications:

The implants of the Foot and Hand Motion are intended for the fixation of bone fractures and osteotomies, and for arthrodeses of the foot and hand in adults.


Contra-indications:

- Pregnancy.
- Acute or chronic local or systemic infections.
- Allergy to one of the materials used or sensitivity to foreign bodies.

*Sterile instrumentation for use with Stand-Alone Screws - Handmotion range. Available separately.



Example of instrumentation kit content for Ø3.0 mm screws

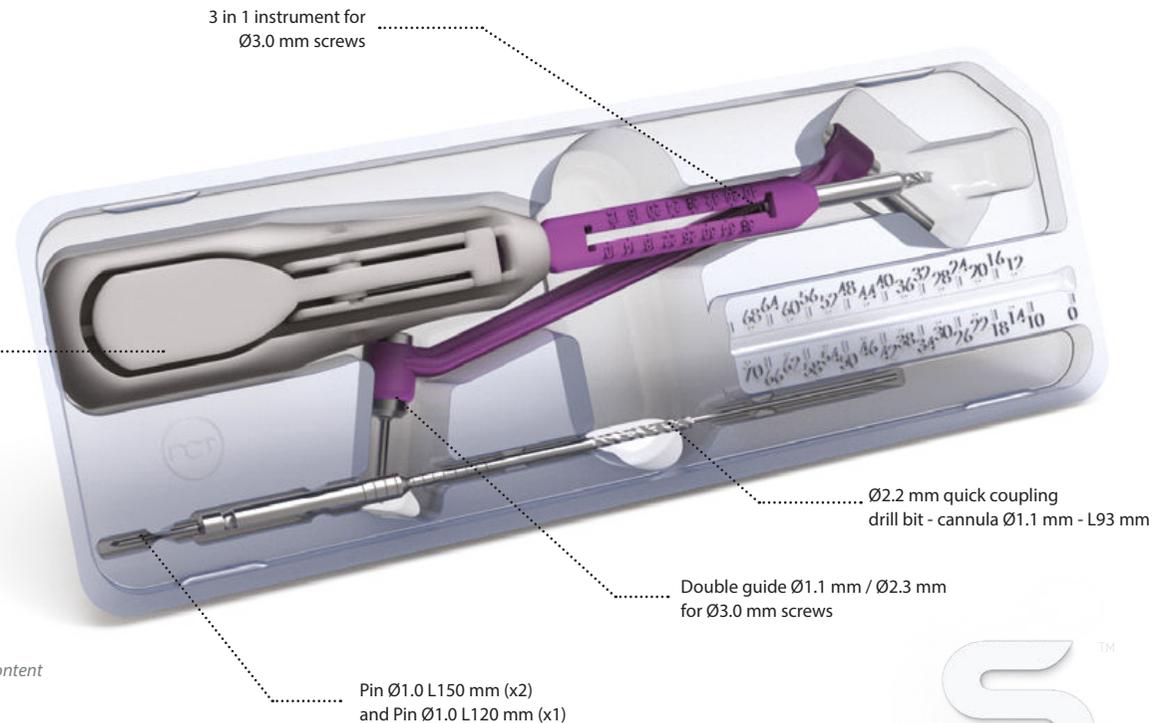

NEWCLIP-TECHNICS



Initial S™: Single use sterile kits for hand surgery

Initial S™ - Hand - Implant references*

*Sterile instrumentation for use with Stand-Alone Screws - Handmotion range. Available separately.

Ø2.25 MM CANNULATED SCREWS

| Ref. | Description |
|-------------------|---|
| H0.9IFT2.25L14-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L14 mm - STERILE |
| H0.9IFT2.25L16-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L16 mm - STERILE |
| H0.9IFT2.25L18-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L18 mm - STERILE |
| H0.9IFT2.25L20-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L20mm - STERILE |
| H0.9IFT2.25L22-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L22 mm - STERILE |
| H0.9IFT2.25L24-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L24 mm - STERILE |
| H0.9IFT2.25L26-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L26 mm - STERILE |
| H0.9IFT2.25L28-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L28 mm - STERILE |
| H0.9IFT2.25L30-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L30 mm - STERILE |
| H0.9IFT2.25L32-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L32 mm - STERILE |
| H0.9IFT2.25L34-ST | Self-drilling self-compressive screw - Ø2.25 mm - cannulated Ø0.9 mm - L34 mm - STERILE |



Ø2.6 MM CANNULATED SCREWS

| Ref. | Description |
|------------------|--|
| H1.1IFT2.6L14-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L14 mm - STERILE |
| H1.1IFT2.6L16-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L16 mm - STERILE |
| H1.1IFT2.6L18-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L18 mm - STERILE |
| H1.1IFT2.6L20-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L20 mm - STERILE |
| H1.1IFT2.6L22-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L22 mm - STERILE |
| H1.1IFT2.6L24-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L24 mm - STERILE |
| H1.1IFT2.6L26-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L26 mm - STERILE |
| H1.1IFT2.6L28-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L28 mm - STERILE |
| H1.1IFT2.6L30-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L30mm - STERILE |
| H1.1IFT2.6L32-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L32 mm - STERILE |
| H1.1IFT2.6L34-ST | Self-drilling self-compressive screw - Ø2.6 mm - cannulated Ø1.1 mm - L34 mm - STERILE |



Ø3.0 MM CANNULATED SCREWS

| Ref. | Description |
|------------------|--|
| H1.1IFT3.0L14-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L14 mm - STERILE |
| H1.1IFT3.0L16-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L16 mm - STERILE |
| H1.1IFT3.0L18-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L18mm - STERILE |
| H1.1IFT3.0L20-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L20 mm - STERILE |
| H1.1IFT3.0L22-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L22 mm - STERILE |
| H1.1IFT3.0L24-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L24 mm - STERILE |
| H1.1IFT3.0L26-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L26 mm - STERILE |
| H1.1IFT3.0L28-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L28 mm - STERILE |
| H1.1IFT3.0L30-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L30 mm - STERILE |
| H1.1IFT3.0L32-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L32 mm - STERILE |
| H1.1IFT3.0L34-ST | Self-drilling self-compressive screw - Ø3.0 mm - cannulated Ø1.1 mm - L34 mm - STERILE |



The information presented in this brochure is intended to demonstrate a Newclip Technics product. Always refer to the package insert, product label and/or user instructions before using any Newclip Technics product. Surgeons must always rely on their own clinical judgment when deciding which products and techniques to use with their patients. Products may not be available in all markets. Product availability is subject to the regulatory or medical practices that govern individual markets. Please contact your Newclip Technics representative if you have questions about the availability of Newclip Technics products in your area.



NEWCLIP TECHNICS (HQ)
PA de la Lande Saint Martin
45 rue des Garottières
44115 Haute Goulaine, France
+33 (0)2 28 21 23 25
orders@newcliptechnics.com
www.newcliptechnics.com

NEWCLIP TECHNICS USA
Newclip USA
642 Larkfield Center
Santa Rosa CA 95403, USA
+1 707 230 5078
customerservice@newclipusa.com
www.newclipusa.com

NEWCLIP TECHNICS IBERIA
Calle Frederic Mompou 4b
Sant Just Desvern
08960 Barcelona, España
+34 938 299 526
contact@newclipiberia.com
www.newcliptechnics.com

NEWCLIP TECHNICS GERMANY
Newclip GmbH
Pröllstraße 11
D-86157 Augsburg, Deutschland
+49 (0)821 650 749 40
info@newclipgmbh.com
www.newclipgmbh.de

NEWCLIP TECHNICS JAPAN
Newclip Technics Japan K.K.
KKK Bldg. 502, 3-18-1 Asakusabashi
Taito-Ku, Tokyo, 111-0053, Japan
+81 (0)3 58 25 49 81
Fax: +81 (0)3 58 25 49 86
www.newcliptechnics.com

NEWCLIP TECHNICS AUSTRALIA
Newclip Australia
3B/11 Donkin Street
West End 4101, Australia
+61 (0)2 81 886 110
solutions@newclipaustralia.com
www.newcliptechnics.com